





- o **Serum Samples:** Use a serum separator tube. Let samples clot at room temperature for 30 minutes before centrifugation for 20 minutes at 1,000xg. Assay freshly prepared serum or store serum in aliquot at  $\leq -20^{\circ}\text{C}$  for later use. Avoid repeated freeze/thaw cycles.
- o **Plasma:** Collect plasma using heparin, EDTA, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000xg within 30 minutes of collection. Assay freshly prepared plasma or store plasma sample in aliquot at  $\leq -20^{\circ}\text{C}$  for later use. Avoid repeated freeze/ thaw cycles.
- o **Urine:** Aseptically collect the urine of the day, voided directly into a sterile container. Assay immediately or aliquot and store at  $\leq -20^{\circ}\text{C}$ . Avoid repeated freeze/thaw cycles.
- o **Serum, Plasma, Urine, Cell Culture Supernatant** have to be diluted in ELISA Buffer 1X. Samples containing visible precipitates must be clarified before use.  
**NOTE:** As a starting point, 1/40,000 dilution of serum and 1/100 dilution of urine are recommended! If sample values fall outside the detection range of the assay, a lower or higher dilution may be required.

**VII. Assay Protocol:**


- Determine the number of 16-well strips needed for the assay and insert them in the frame for current use. The extra strips should be resealed in the foil pouch bag and stored at  $4^{\circ}\text{C}$ .  
**NOTE:** Remaining 16-well strips coated with RPB4 antibody when opened can be stored at  $4^{\circ}\text{C}$  for up to 1 month.
- Add 100  $\mu\text{l}$  of the different **standards** into the appropriate wells in duplicate. At the same time, add 100  $\mu\text{l}$  of **diluted serum, plasma, urine, cell culture supernatant** samples in duplicate to the wells. Cover the plate with plate sealer and incubate for 1 hour at  $37^{\circ}\text{C}$ .
- Aspirate the coated wells and add 300  $\mu\text{l}$  of **Wash Buffer 1X** using a multichannel pipette or auto-washer. Repeat the process for a total of three washes. After the last wash, complete removal of liquid is essential for good performance.
- Add 100  $\mu\text{l}$  to each well of the **Detection Antibody**. Cover the plate with plate sealer and incubate for 1 hour at  $37^{\circ}\text{C}$ .
- Aspirate the coated wells and add 300  $\mu\text{l}$  of **Wash Buffer 1X** using a multichannel pipette or auto-washer. Repeat the process for a total of three washes. After the last wash, complete removal of liquid is essential for good performance.
- Add 100  $\mu\text{l}$  to each well of the diluted **HRP**. Cover the plate with plate sealer and incubate for 1 hour at  $37^{\circ}\text{C}$ .
- Aspirate the coated wells and add 300  $\mu\text{l}$  of **Wash Buffer 1X** using a multichannel pipette or auto-washer. Repeat the process for a total of five washes. After the last wash, complete removal of liquid is essential for good performance.
- Add 100  $\mu\text{l}$  to each well of **TMB Substrate Solution**. Allow the color reaction to develop at room temperature in the dark for 20 minutes.
- Stop the reaction by adding 100  $\mu\text{l}$  of **Stop Solution**. Tap the plate gently to ensure thorough mixing. The substrate reaction yields a blue solution that turns yellow when Stop Solution is added.
- Measure the OD at 450 nm in an ELISA reader within 30 minutes.

**VIII. Calculation of Results:**

- Average the duplicate readings for each standard, control and sample and subtract the average blank value (obtained with the 0 ng/ml point).
- Generate the standard curve by plotting the average absorbance obtained for each standard concentration on the horizontal (X) axis vs. the corresponding RBP4 concentration (ng/ml) on the vertical (Y) axis (see Typical Data).
- Calculate the RBP4 concentrations of samples by interpolation of the regression curve formula as shown above in a form of a quadratic equation.
- If the test samples were diluted, multiply the interpolated values by the dilution factor to calculate the concentration of human RBP4 in the samples.

**IX. Typical Data:**

The following data are obtained using the different concentrations of standard as described in this protocol:

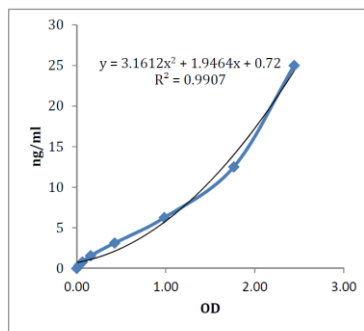

Standard hRBP4 (ng/ml)	Optical Density (mean)
25	2.44
12.5	1.76
6.25	0.98
3.13	0.43
1.56	0.16
0.78	0.06
0.39	0.03
0	0.00

Figure: Standard curve

**X. RELATED PRODUCTS:**

- |                                          |                                      |
|------------------------------------------|--------------------------------------|
| RBP4, Human recombinant                  | RBP4, Rat recombinant                |
| RBP4, Mouse recombinant                  | Recombinant proteins and enzymes     |
| ELISA kits                               | Metabolism Assay kits and Reagents   |
| Apoptosis Assay Kits and Reagents        | Cellular Fractionation Kits          |
| Recombinant Growth Factors and Cytokines | Polyclonal and monoclonal antibodies |

**FOR RESEARCH USE ONLY! Not to be used on humans.**