

α-Ketoglutarate Colorin

(Catalog #K677-100; 100 assays; Store Kit at -20°C)

I. Introduction:

α-Ketoglutarate (α-KG) is a key intermediate in the Krebs cycle, coming after isocitrate and before succinyl CoA. Anaplerotic reactions replenish the cycle by synthesizing α-KG from transamination of glutamate, or through the action of glutamate dehydrogenase. α-KG is an important nitrogen transporter. Being a key intermediate, it is one of the organic acids measured in newborns as an indicator of inborn errors of metabolism. BioVision's α-Ketoglutarate Assay Kit provides a simple, sensitive and rapid means for quantifying α-KG in a variety of samples. In the assay, α-ketoglutarate is transaminated with the generation of pyruvate which is utilized to convert a nearly colorless probe to both color ($\lambda_{max} = 570\text{nm}$) and fluorescence (Ex/Em = 535/587 nm). The α-Ketoglutarate Assay Kit is useful for detecting α-ketoglutarate in the range of 0.01 to 10 nmoles.

II. Kit Contents:

Components	K677-100	Cap Code	Part Number
α-KG Assay Buffer	25 ml	WM	K677-100-1
α-KG OxiRed Probe (in DMSO)	0.2 ml	Red	K677-100-2A
α-KG Converting Enzyme (lyophilized)	1 vial	Purple	K677-100-4
α-KG Development Enzyme Mix (lyophilized)	1 vial	Green	K677-100-5
α-KG Standard (10 μmol, lyophilized)	1 vial	Yellow	K677-100-6

III. Storage and Handling:

Store kit at -20°C, protect from light. Warm α-KG Assay Buffer to room temperature before use. Briefly centrifuge all small vials prior to opening.

IV. Reagent Preparation and Storage Conditions:

α-KG Probe: Ready to use as supplied. Warm to room temperature before using to melt frozen DMSO. Protect from light and moisture. Stable for 2 months at -20°C.

α-KG Converting Enzyme, α-KG Enzyme Mix: Dissolve with 220 μl α-KG Buffer separately. Pipette up and down to dissolve. Aliquot into vials with sufficient amount for each experiment and store at -20°C. Avoid repeated freeze/thaw cycles. Use within two months.

α-KG Standard: Dissolve in 100 μl dH₂O to generate 100 mM (100nmol/μl) α-KG Standard solution. Keep cold while in use. Store at -20°C.

V. Assay Protocol:

1. Standard Curve Preparations:

Dilute the α-KG Standard to 1 nmol/μl by adding 10 μl of the Standard to 990 μl of dH₂O, mix well. Add 0, 2, 4, 6, 8, 10 μl into a series of standards wells on a 96-well plate. Adjust volume to 50 μl/well with Assay Buffer to generate 0, 2, 4, 6, 8, 10 nmol/well of the Standard.

Fluorometric Assay: Dilute further dilute by adding 10 μl to 90 μl of dH₂O. Add 0, 2, 4, 6, 8, 10 μl into a series of standards well on a 96-well plate. Adjust the volume to 50 μl/well to generate 0, 0.2, 0.4, 0.6, 0.8, 1.0 nmol/well.

2. Sample Preparation:

Tissue (20 mg) or cells (2×10^6) are rapidly homogenized with 100 μl of ice cold α-KG Assay Buffer. Enzymes in samples may interfere with the assay. We suggest deproteinizing samples using a perchloric acid/KOH protocol (BioVision, Cat.#K808-200) or 10 kDa molecular weight cut off spin columns (BioVision, Cat# 1997-25). Add 1 - 50 μl samples into duplicate wells of a 96-well plate and bring volume to 50 μl with Assay Buffer. We suggest testing several doses of your samples to ensure readings are within the linear range.

- Mix enough reagent for the number of samples and standards to be performed: For each well, prepare a total 50 μl Reaction Mix containing:

	Sample	Bkgd. Control*
α-KG Assay Buffer	44 μl	46 μl
α-KG Converting Enzyme	2 μl	-----
α-KG Enzyme Mix	2 μl	2 μl
α-KG probe	2 μl	2 μl

Add 50 μl of the Reaction Mix to each well containing the α-KG Standard, samples or background control*.

***Note1:** Pyruvate generates background. If pyruvate is suspected in your sample, you can do the background control omitting the converting enzyme. The background control can be subtracted from the α-KG reading.

Note2 (optional): for fluorometric assay use 0.4 μl α-KG OxiRed Probe and 45.6 μl (47.6 μl for Bkgd Control) α-KG assay buffer to reduce background



- Incubate for 30 min at 37°C, protect from light.
- Measure OD at 570 nm or fluorescence using Ex/Em = 535/587 nm.
- Calculation:** Correct background by subtracting the value of the 0 α-KG blank from all readings. Plot the standard curve. Apply the corrected sample readings to the standard curve to get α-KG amount in the sample wells. The α-KG concentrations in the test samples:

$$C = Ay/Sv \text{ (nmol/}\mu\text{l; or } \mu\text{mol/ml; or mM)}$$

Where: Ay is the amount of α-KG (nmol) in your sample from the standard curve.

Sv is the sample volume (μl) added to the sample well.

α-Ketoglutarate molecular weight: 146.11

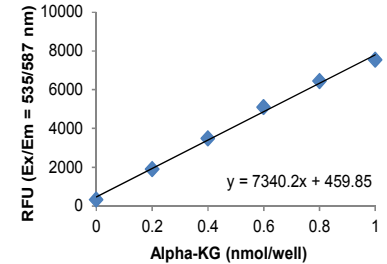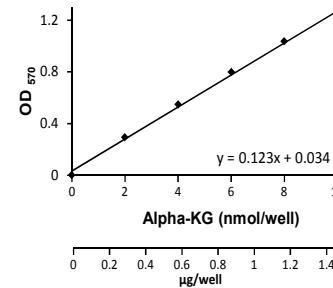

α-Ketoglutarate standard curve generated using this kit protocol.

RELATED PRODUCTS:

- Apoptosis Detection Kits & Reagents
- Glucose, Sucrose Assay Kit
- Glutathione Assay Kit
- NAD/NADH and NADP/NADPH Assay Kit
- TAC Total Antioxidant Capacity
- Malic acid Assay Kit
- Glycogen Assay Kit
- Galactose Assay Kit
- Fructose Assay Kit

- Cell Proliferation & Senescence Kits
- Cholesterol, LDL/HDL Assay Kits
- Ethanol and Uric Acid Assay Kit
- Lactate Assay Kits
- Mono or Polysaccharide Assay Kits
- Pyruvate Assay Kit
- Fatty Acid Assay Kit
- Nitric Oxide Assay Kit
- Iron Assay Kit

FOR RESEARCH USE ONLY! Not to be used on humans.

GENERAL TROUBLESHOOTING GUIDE:

Problems	Cause	Solution
Assay not working	<ul style="list-style-type: none"> • Use of ice-cold assay buffer • Omission of a step in the protocol • Plate read at incorrect wavelength • Use of a different 96-well plate 	<ul style="list-style-type: none"> • Assay buffer must be at room temperature • Refer and follow the data sheet precisely • Check the wavelength in the data sheet and the filter settings of the instrument • Fluorescence: Black plates (clear bottoms) ; Luminescence: White plates ; Colorimeters: Clear plates
Samples with erratic readings	<ul style="list-style-type: none"> • Use of an incompatible sample type • Samples prepared in a different buffer • Samples were not deproteinized (if indicated in datasheet) • Cell/ tissue samples were not completely homogenized • Samples used after multiple free-thaw cycles • Presence of interfering substance in the sample • Use of old or inappropriately stored samples 	<ul style="list-style-type: none"> • Refer data sheet for details about incompatible samples • Use the assay buffer provided in the kit or refer data sheet for instructions • Use the 10 kDa spin cut-off filter or PCA precipitation as indicated • Use Dounce homogenizer (increase the number of strokes); observe for lysis under microscope • Aliquot and freeze samples if needed to use multiple times • Troubleshoot if needed, deproteinize samples • Use fresh samples or store at correct temperatures till use
Lower/ Higher readings in Samples and Standards	<ul style="list-style-type: none"> • Improperly thawed components • Use of expired kit or improperly stored reagents • Allowing the reagents to sit for extended times on ice • Incorrect incubation times or temperatures • Incorrect volumes used 	<ul style="list-style-type: none"> • Thaw all components completely and mix gently before use • Always check the expiry date and store the components appropriately • Always thaw and prepare fresh reaction mix before use • Refer datasheet & verify correct incubation times and temperatures • Use calibrated pipettes and aliquot correctly
Readings do not follow a linear pattern for Standard curve	<ul style="list-style-type: none"> • Use of partially thawed components • Pipetting errors in the standard • Pipetting errors in the reaction mix • Air bubbles formed in well • Standard stock is at an incorrect concentration • Calculation errors • Substituting reagents from older kits/ lots 	<ul style="list-style-type: none"> • Thaw and resuspend all components before preparing the reaction mix • Avoid pipetting small volumes • Prepare a master reaction mix whenever possible • Pipette gently against the wall of the tubes • Always refer the dilutions in the data sheet • Recheck calculations after referring the data sheet • Use fresh components from the same kit
Unanticipated results	<ul style="list-style-type: none"> • Measured at incorrect wavelength • Samples contain interfering substances • Use of incompatible sample type • Sample readings above/below the linear range 	<ul style="list-style-type: none"> • Check the equipment and the filter setting • Troubleshoot if it interferes with the kit • Refer data sheet to check if sample is compatible with the kit or optimization is needed • Concentrate/ Dilute sample so as to be in the linear range
<p>Note: The most probable list of causes is under each problem section. Causes/ Solutions may overlap with other problems.</p>		